

# Alcotest 7110 Calibration Record

## Equipment

Alcotest 7110 MKIII-C  
Serial No.: ARTL-0014  
Location: SOUTH BRUNSWICK POLICE  
Calibration File No.: 00210 Calib. Date: 01/06/2009 Calib. No.: 00009  
Certification File No.: 00201 Cert. Date: 08/15/2008 Cert. No.: 00006  
Linearity File No.: 00202 Lin. Date: 08/15/2008 Lin. No.: 00006  
Solution File No.: 00209 Soln. Date: 12/24/2008 Soln. No.: 00053  
Sequential File No.: 00210 File Date: 01/06/2009

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUH S3-0079  
Control Solution %: 0.100% Expires: 07/02/2010  
Solution Control Lot: 08G056 Bottle No.: 0710


## Coordinator

Last Name: SNYDER First Name: THOMAS MI: J.

Signature: THOMAS J. SNYDER #5792 Badge No.: 5792  
Date: 01/06/2009

\*Black Key Temperature Probe Serial .....# DDUH P2 - 229 592

\*Ertco-Hart Digital Temperature Measuring System Serial# A29881 592

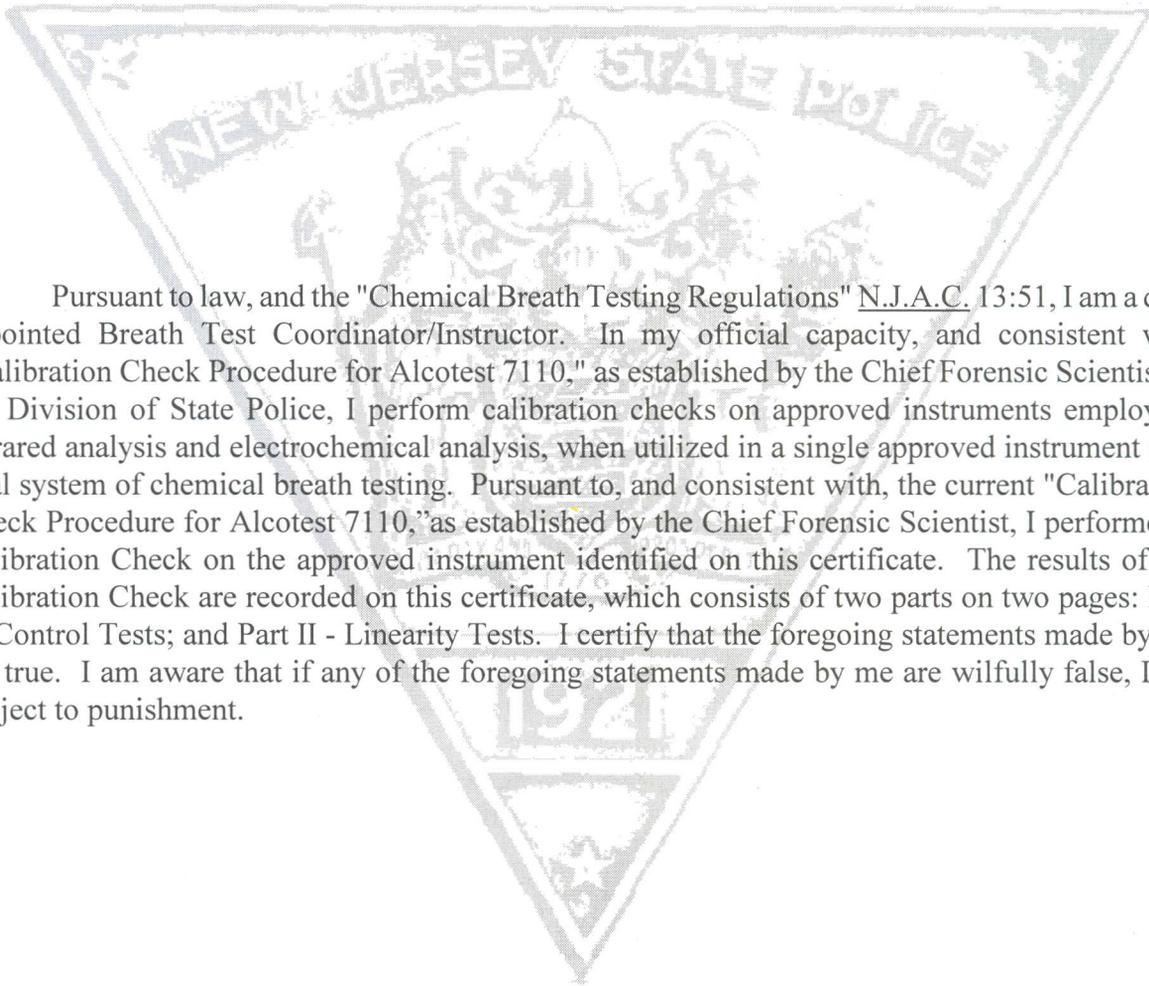

Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis, when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to, and consistent with, the current "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.

# Alcotest 7110 Calibration Certificate

## Part I - Control Tests

**Equipment** Alcotest 7110 MKIII-C Serial No.: ARTL-0014  
Location: SOUTH BRUNSWICK POLICE  
Calibration File No.: 00210 Calib. Date: 01/06/2009 Calib. No.: 00009  
Certification File No.: 00211 Cert. Date: 01/06/2009 Cert. No.: 00007  
Linearity File No.: 00202 Lin. Date: 08/15/2008 Lin. No.: 00006  
Solution File No.: 00209 Soln. Date: 12/24/2008 Soln. No.: 00053  
Sequential File No.: 00211 File Date: 01/06/2009

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUH S3-0079  
Control Solution %: 0.100% Expires: 07/02/2010  
Solution Control Lot: 08G056 Bottle No.: 0710

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	10:35S		
Control 1 EC	0.099%	10:35S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	10:35S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:36S		
Control 2 EC	0.098%	10:37S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	10:37S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:38S		
Control 3 EC	0.099%	10:38S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	10:38S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:39S		

All tests within acceptable tolerance.

### Coordinator

Last Name: SNYDER

First Name: THOMAS

MI: J.

Badge No.: 5792

Date: 01/06/2009

Signature: TPR. I Thomas J. Snyder #5792

Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis, when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to, and consistent with, the current "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.

# Alcotest 7110 Calibration Certificate

## Part II - Linearity Tests

**Equipment** Alcotest 7110 MKIII-C Serial No.: ARTL-0014  
Location: SOUTH BRUNSWICK POLICE  
Calibration File No.: 00210 Calib. Date: 01/06/2009 Calib. No.: 00009  
Certification File No.: 00211 Cert. Date: 01/06/2009 Cert. No.: 00007  
Linearity File No.: 00212 Lin. Date: 01/06/2009 Lin. No.: 00007  
Solution File No.: 00209 Soln. Date: 12/24/2008 Soln. No.: 00053  
Sequential File No.: 00212 File Date: 01/06/2009

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDRK S3-0003  
Control Solution %: 0.040% Expires: 06/26/2010  
Solution Control Lot: 08F054 Bottle No.: 0168

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDXD S3-0184  
Control Solution %: 0.080% Expires: 06/28/2010  
Solution Control Lot: 08F055 Bottle No.: 0345

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDSC S3-0009  
Control Solution %: 0.160% Expires: 07/07/2010  
Solution Control Lot: 08G057 Bottle No.: 1395

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	10:55S		
Control 1 EC	0.042%	10:55S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.041%	10:55S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:57S		
Control 2 EC	0.041%	10:58S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.039%	10:58S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:59S		
Control 3 EC	0.082%	11:00S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.080%	11:00S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:01S		
Control 4 EC	0.081%	11:02S	34.0°C	*** TEST PASSED ***
Control 4 IR	0.079%	11:02S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:04S		
Control 5 EC	0.161%	11:04S	33.9°C	*** TEST PASSED ***
Control 5 IR	0.160%	11:04S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:06S		
Control 6 EC	0.160%	11:06S	33.9°C	*** TEST PASSED ***
Control 6 IR	0.159%	11:06S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:08S		

All tests within acceptable tolerance.

### Coordinator

Last Name: SNYDER

First Name: THOMAS

MI: J.

Signature: TPR. I Thomas J. Snyder # 5792

Badge No.: 5792

Date: 01/06/2009

# Calibrating Unit

## New Standard Solution Report

**Equipment** Alcotest 7110 MKIII-C Serial No.: ARTL-0014  
Location: SOUTH BRUNSWICK POLICE  
Calibration File No.: 00210 Calib. Date: 01/06/2009 Calib. No.: 00009  
Certification File No.: 00211 Cert. Date: 01/06/2009 Cert. No.: 00007  
Linearity File No.: 00212 Lin. Date: 01/06/2009 Lin. No.: 00007  
Solution File No.: 00213 Soln. Date: 01/06/2009 Soln. No.: 00054  
Sequential File No.: 00213 File Date: 01/06/2009

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUH S3-0079  
Control Solution %: 0.100% Expires: 10/03/2009  
Solution Control Lot: 07J048 Bottle No.: 1387

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	12:22S		
Control 1 EC	0.101%	12:22S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	12:22S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:23S		
Control 2 EC	0.099%	12:24S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	12:24S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:25S		
Control 3 EC	0.100%	12:25S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	12:25S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:26S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

TEMPERATURE PROBE SERIAL NUMBER: DJSFP2-0394 (594)

### Changed By:

Last Name: SNYDER

First Name: THOMAS

MI: J.

Signature: THOMAS J. SNYDER #5792

Badge No.: 5792

Date: 01/06/2009



Dräger safety

# CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.  
(F.R. Vol. 59 No. 249 12/19/94 Notices)

**Draeger Safety Diagnostics, Inc.**

- Model: ALCOTEST® CU34
- Model: MARK IIA
- Other: \_\_\_\_\_

Serial Number:

DDRK 53-0003

Certification Date

Technician

Re-Certification Due Date

02-13-08

*[Signature]*

02-13-09



Dräger safety

# CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.  
(F.R. Vol. 59 No. 249 12/19/94 Notices)

**Draeger Safety Diagnostics, Inc.**

- Model: ALCOTEST® CU34
- Model: MARK IIA
- Other: \_\_\_\_\_

Serial Number:

DDXDS3-0184

Certification Date

Technician

Re-Certification Due Date

02-13-08

*[Signature]*

02-13-09



Dräger safety

# CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.  
(F.R. Vol. 59 No. 249 12/19/94 Notices)

**Draeger Safety Diagnostics, Inc.**

- Model: ALCOTEST® CU34
- Model: MARK IIA
- Other: \_\_\_\_\_

Serial Number:

DDSC 33-0009

Certification Date

Technician

Re-Certification Due Date

02-13-08

02-13-09

## Dräger safety

### ALCOTEST® 7110 TEMPERATURE PROBE

# CERTIFICATE OF ACCURACY

This is to certify that the Alcotest® 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST). The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your State Specification. For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest® 7110.

Serial Number Temp. Probe

Certification date:

Next Certification due:

DDUAP2-229

02-12-08

02-12-09

Probe Value

102

**Draeger Safety Diagnostics, Inc.**  
Technical Service Department

**Dräger**safety

Ertco-Hart Digital Temperature Measuring System

**REPORT OF CALIBRATION**

This is to certify that the Ertco-Hart Digital Temperature Measuring System has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST). Draeger Safety Diagnostics, Inc. (DSDI) recommends accuracy verification of the Ertco-Hart Digital Temperature Measuring System within 12 months of the certification date below, or sooner, according to your state specification.

DSDI equipment used for temperature verification Serial Number: HH41 301316 / HH41 303176 / MERCURY THERMOMETER

Digital Units Serial Number: A29881

Probe Serial Number: 590802

Certification Date: 02-12-2008

Next Certification Due: 02-12-2009

At 34.00 °C digital unit displays 34.06 °C

Draeger Safety Diagnostics, Inc. Technician: 



State of New Jersey  
 OFFICE OF THE ATTORNEY GENERAL  
 DEPARTMENT OF LAW AND PUBLIC SAFETY  
 DIVISION OF STATE POLICE  
 POST OFFICE BOX 7068  
 WEST TRENTON NJ 08628-0068  
 (609) 882-2000

JON S. CORZINE  
 Governor

ANNE MILGRAM  
 Attorney General

COLONEL JOSEPH R. FUENTES  
 Superintendent

**CERTIFICATION OF ANALYSIS**  
**0.10 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION**

**ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION:** Ethyl alcohol concentration within, but not exceeding, the range of 0.117 to 0.125 grams per 100 milliliters of solution.

**MANUFACTURER:** Drager Safety, Inc.      **ANALYSIS DATE:** 07/24/2008

**BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER:** 08G056

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have an ethyl alcohol concentration range of 0.1227 to 0.1236 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is July 2, 2010.

As Chief Forensic Scientist of the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at my direction and under my supervision by personnel of, and at, the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Ajit R. Tungare  
 Chief Forensic Scientist  
 Division of State Police

Sworn to and subscribed before me this 13<sup>th</sup> day of August, 2008.

Notary

**Linda L. DeSantis**  
**My Commission**  
**Expires Aug. 17, 2009**



New Jersey Is An Equal Opportunity Employer  
 Printed on Recycled Paper and Recyclable





State of New Jersey  
 OFFICE OF THE ATTORNEY GENERAL  
 DEPARTMENT OF LAW AND PUBLIC SAFETY  
 DIVISION OF STATE POLICE  
 POST OFFICE BOX 7068  
 WEST TRENTON NJ 08628-0068  
 (609) 882-2000

JON S. CORZINE  
 Governor

ANNE MILGRAM  
 Attorney General

COLONEL JOSEPH R. FUENTES  
 Superintendent

**CERTIFICATION OF ANALYSIS**  
**0.040 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION**

**ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION:** Ethyl alcohol concentration within, but not exceeding, the range of 0.045 to 0.051 grams per 100 milliliters of solution.

**MANUFACTURER:** Drager Safety, Inc.      **ANALYSIS DATE:** 07/16/2008

**BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER:** 08F054

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have an ethyl alcohol concentration range of 0.0487 to 0.0493 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is June 26, 2010.

As Chief Forensic Scientist of the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at my direction and under my supervision by personnel of, and at, the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Ajit R. Tungare  
 Chief Forensic Scientist  
 Division of State Police

Sworn to and subscribed before me this 19<sup>th</sup> day of August, 2008.

Notary

JOHN R. LEAVER  
 NOTARY PUBLIC STATE OF NEW JERSEY  
 MY COMMISSION EXPIRES 12/14/2012



New Jersey Is An Equal Opportunity Employer  
 Printed on Recycled Paper and Recyclable





State of New Jersey  
 OFFICE OF THE ATTORNEY GENERAL  
 DEPARTMENT OF LAW AND PUBLIC SAFETY  
 DIVISION OF STATE POLICE  
 POST OFFICE BOX 7068  
 WEST TRENTON NJ 08628-0068  
 (609) 882-2000

JON S. CORZINE  
 Governor

ANNE MILGRAM  
 Attorney General

COLONEL JOSEPH R. FUENTES  
 Superintendent

**CERTIFICATION OF ANALYSIS**  
**0.080 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION**

**ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION:** Ethyl alcohol concentration within, but not exceeding, the range of 0.094 to 0.099 grams per 100 milliliters of solution.

**MANUFACTURER:** Drager Safety, Inc.      **ANALYSIS DATE:** 07/25/2008

**BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER:** 08F055

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have an ethyl alcohol concentration range of 0.0977 to 0.0984 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is June 28, 2010.

As Chief Forensic Scientist of the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at my direction and under my supervision by personnel of, and at, the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Ajit R. Tungare  
 Chief Forensic Scientist  
 Division of State Police

Sworn to and subscribed before me this 19<sup>th</sup> day of August, 2008.

Notary

JOHN R. LEAVER  
 NOTARY PUBLIC STATE OF NEW JERSEY  
 MY COMMISSION EXPIRES 12/14/2012



New Jersey Is An Equal Opportunity Employer  
 Printed on Recycled Paper and Recyclable





State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON NJ 08628-0068
(609) 882-2000

JON S. CORZINE
Governor

ANNE MILGRAM
Attorney General

COLONEL JOSEPH R. FUENTES
Superintendent

CERTIFICATION OF ANALYSIS
0.160 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.188 to 0.199 grams per 100 milliliters of solution.

MANUFACTURER: Drager Safety, Inc. ANALYSIS DATE: 07/28/2008

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 08G057

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have an ethyl alcohol concentration range of 0.1956 to 0.1959 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is July 7, 2010.

As Chief Forensic Scientist of the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at my direction and under my supervision by personnel of, and at, the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Ajit R. Tungare (Handwritten signature)

Ajit R. Tungare
Chief Forensic Scientist
Division of State Police

Sworn to and subscribed before me this 19th day of August, 2008.

(Handwritten signature of John R. Leaver)
Notary

JOHN R. LEAVER
NOTARY PUBLIC STATE OF NEW JERSEY
MY COMMISSION EXPIRES 12/14/2012



New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable





State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON NJ 08628-0068
(609) 882-2000

JON S. CORZINE
Governor

ANNE MILGRAM
Attorney General

COLONEL JOSEPH R. FUENTES
Superintendent

CERTIFICATION OF ANALYSIS
0.10 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.117 to 0.125 grams per 100 milliliters of solution.

MANUFACTURER: Drager Safety, Inc. ANALYSIS DATE: 11/28/07

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 07J048

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have an ethyl alcohol concentration range of 0.1225 to 0.1229 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is October 3, 2009.

As Chief Forensic Scientist of the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at my direction and under my supervision by personnel of, and at, the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

[Handwritten signature of Ajit R. Tungare]

Ajit R. Tungare
Chief Forensic Scientist
Division of State Police

Sworn to and subscribed before me this 17th day of December, 2007.

[Handwritten signature of Linda L. DeSantis]
Notary

Linda L. DeSantis
My Commission
Expires Aug. 17, 2009



New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable



DEPARTMENT OF  
**Traffic and Public Safety**  
This is to certify that

**Thomas J. Snyder**  
New Jersey State Police

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL BREATH ANALYSES PURSUANT TO CHAPTER 142 OF THE LAWS OF 1966 IN THE OPERATION OF THE ALCOTEST 7110 MKIII-C A METHOD TO DETERMINE INTOXICATION.

GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY THIS 22nd DAY OF February  
TWO THOUSAND AND SIX

*Joseph P. ...*  
SUPERINTENDENT  
NEW JERSEY STATE POLICE

*Julian V. ...*  
ATTORNEY GENERAL  
STATE OF NEW JERSEY

ORIGINAL COURSE DATES \_\_\_\_\_

DATE	Refresher Course PLACE	INSTRUCTOR
1. 03/27/08	SUSSEX F.A.	M. ...
2. _____	_____	_____
3. _____	_____	_____
4. _____	_____	_____
5. _____	_____	_____
6. _____	_____	_____
7. _____	_____	_____
8. _____	_____	_____
9. _____	_____	_____

S.P. 293B (Rev. 01/06)

DEPARTMENT OF  
**Traffic and Public Safety**  
This is to certify that

**Thomas J. Snyder**  
Breath Test Coordinator/Instructor

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL BREATH ANALYSES PURSUANT TO CHAPTER 142 OF THE LAWS OF 1966 IN THE OPERATION OF THE Alcotest 7110 MKIII-C A METHOD TO DETERMINE INTOXICATION.

GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY THIS 17th DAY OF June  
TWO THOUSAND AND SIX

*Joseph P. ...*  
SUPERINTENDENT  
NEW JERSEY STATE POLICE

*Julian V. ...*  
ATTORNEY GENERAL  
STATE OF NEW JERSEY

ORIGINAL COURSE DATES \_\_\_\_\_

DATE	Refresher Course PLACE	INSTRUCTOR
1. 03/27/08	SUSSEX F.A.	M. ...
2. _____	_____	_____
3. _____	_____	_____
4. _____	_____	_____
5. _____	_____	_____
6. _____	_____	_____
7. _____	_____	_____
8. _____	_____	_____
9. _____	_____	_____

S.P. 293B (Rev. 01/06)

DEPARTMENT OF  
**Traffic and Public Safety**  
This is to certify that

**Thomas J. Snyder**  
New Jersey State Police

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL BREATH ANALYSES PURSUANT TO CHAPTER 142 OF THE LAWS OF 1966 IN THE OPERATION OF THE Breathalyzer A METHOD TO DETERMINE INTOXICATION.

GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY THIS 11th DAY OF Aug.  
TWO THOUSAND AND 00

*Gene ...*  
SUPERINTENDENT  
NEW JERSEY STATE POLICE

*...*  
ATTORNEY GENERAL  
STATE OF NEW JERSEY

ORIGINAL COURSE DATES \_\_\_\_\_

DATE	Refresher Course PLACE	INSTRUCTOR
1. 11-14-04	ACTC	M. ...
2. 5-5-03	OLPA	...
3. 4-4-05	ACTC	C. ...
4. 7-26-07	OLPA	C. ...
5. _____	_____	_____
6. _____	_____	_____
7. _____	_____	_____
8. _____	_____	_____
9. _____	_____	_____

SP-293B (Rev. 11/99)

Drägersafety

Alcotest<sup>®</sup> 7110 MKIII-C

**CERTIFICATE OF ACCURACY**

This is to certify that the Alcotest 7110 MKIII-C has been tested for accuracy and found to be in compliance with the National Highway Traffic Safety Administration Standard for evidential breath testing devices. The Alcotest MKIII-C is compliant as a "mobile" and "nonmobile" EBT with 49 FR 48854, 49 FR 48864 and 58 FR 48705. The manufacturer recommends accuracy verification of this instrument within 12 months of the calibration date below, or sooner, according to your State Specifications.

Certification Date:

04/02/2007

SERIAL NUMBER:

ARTL - 0014

Draeger Safety Diagnostics, Inc.  
Durango, CO

CRD



**Dräger**safety

# CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.  
(F.R. Vol. 59 No. 249 12/19/94 Notices)

**Draeger Safety Diagnostics, Inc.**

- Model: ALCOTEST® CU34
- Model: MARK IIA
- Other: \_\_\_\_\_

Serial Number:

DAUHS3-0079

Certification Date

Technician

Re-Certification Due Date

07-22-08

*[Signature]*

07-22-09

**Dräger**safety

Recreated on  
02/05/2009

ALCOTEST® 7110 TEMPERATURE PROBE

**CERTIFICATE OF ACCURACY**

This is to certify that the Alcotest® 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST). The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your State Specification. For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest® 7110.

Serial Number Temp. Probe

DDSEFP2-0394

Certification date:

07-22-08

Next Certification due:

07-22-09

Probe Value

104

**Draeger Safety Diagnostics, Inc.**  
Technical Service Department

