

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARTL-0014
Location:	SOUTH BRUNSWICK POLICE	
Calibration File No.:	00200	Calib. Date: 08/15/2008
Certification File No.:	00201	Cert. No.: 00008
Linearity File No.:	00202	Cert. Date: 08/15/2008
Solution File No.:	00203	Lin. Date: 08/15/2008
Sequential File No.:	00203	Lin. No.: 00006
		Soln. Date: 08/15/2008
		Soln. No.: 00048
		File Date: 08/15/2008
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUF S3-0060
Solution Control Lot:	08A049	Expires: 01/09/2010
		Bottle No.: 1021

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	10:40D		
Control 1 EC	0.101%	10:40D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	10:40D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:41D		
Control 2 EC	0.100%	10:41D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	10:41D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:42D		
Control 3 EC	0.100%	10:43D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	10:43D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:43D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

TEMPERATURE PROBE SERIAL NUMBER: DJSFP2-0416 JJS

Changed By:

Last Name: SNYDER

First Name: THOMAS

MI: J.

Signature: TPR. I Thomas J. Snyder #5792

Badge No.: 5792

Date: 08/15/2008

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARTL-0014
Location:	SOUTH BRUNSWICK POLICE	
Calibration File No.:	00163	Calib. Date: 09/21/2007
Certification File No.:	00164	Calib. No.: 00007
Linearity File No.:	00165	Cert. Date: 09/21/2007
Solution File No.:	00193	Cert. No.: 00005
Sequential File No.:	00193	Lin. Date: 09/21/2007
		Lin. No.: 00005
		Soln. Date: 07/17/2008
		Soln. No.: 00047
		File Date: 07/17/2008
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUF S3-0060
Solution Control Lot:	08A049	Expires: 01/09/2010
		Bottle No.: 1016

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	03:04D		
Control 1 EC	0.099%	03:04D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	03:04D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	03:05D		
Control 2 EC	0.099%	03:05D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	03:05D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	03:06D		
Control 3 EC	0.100%	03:06D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	03:06D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	03:07D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: ROGERS

First Name: MICHAEL

MI: J

Signature: _____

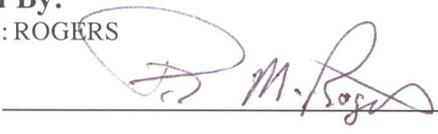

Badge No.: 258

Date: 07/17/2008

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARTL-0014
Location:	SOUTH BRUNSWICK POLICE	
Calibration File No.:	00163	Calib. Date: 09/21/2007
Certification File No.:	00164	Calib. No.: 00007
Linearity File No.:	00165	Cert. Date: 09/21/2007
Solution File No.:	00189	Cert. No.: 00005
Sequential File No.:	00189	Lin. Date: 09/21/2007
		Lin. No.: 00005
		Soln. Date: 06/17/2008
		Soln. No.: 00046
		File Date: 06/17/2008
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUF S3-0060
Solution Control Lot:	07B044	Expires: 02/20/2009
		Bottle No.: 0706

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	15:33D		
Control 1 EC	0.099%	15:33D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	15:33D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:34D		
Control 2 EC	0.099%	15:34D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	15:34D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:35D		
Control 3 EC	0.099%	15:35D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	15:35D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:36D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

TEMPERATURE PROBE SERIAL NUMBER: DDSFP2-0416 TJS

Changed By:

Last Name: SNYDER	First Name: THOMAS	MI: J.
Signature: <u>TR. I Thomas J. Snyder #5792</u>	Badge No.: 5792	Date: 06/17/2008

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTL-0014
Location: SOUTH BRUNSWICK POLICE
Calibration File No.: 00163 Calib. Date: 09/21/2007 Calib. No.: 00007
Certification File No.: 00164 Cert. Date: 09/21/2007 Cert. No.: 00005
Linearity File No.: 00165 Lin. Date: 09/21/2007 Lin. No.: 00005
Solution File No.: 00188 Soln. Date: 05/23/2008 Soln. No.: 00045
Sequential File No.: 00188 File Date: 05/23/2008

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUH S3-0079
Control Solution %: 0.100% Expires: 02/20/2009
Solution Control Lot: 07B044 Bottle No.: 0716

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	13:50D		
Control 1 EC	0.100%	13:50D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.101%	13:50D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:51D		
Control 2 EC	0.099%	13:51D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	13:51D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:52D		
Control 3 EC	0.099%	13:53D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	13:53D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:53D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: ROGERS

First Name: MICHAEL

MI: J

Signature: _____



Badge No.: 258

Date: 05/23/2008

Calibrating Unit New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTL-0014
Location: SOUTH BRUNSWICK POLICE
Calibration File No.: 00163 Calib. Date: 09/21/2007 Calib. No.: 00007
Certification File No.: 00164 Cert. Date: 09/21/2007 Cert. No.: 00005
Linearity File No.: 00165 Lin. Date: 09/21/2007 Lin. No.: 00005
Solution File No.: 00187 Soln. Date: 04/26/2008 Soln. No.: 00044
Sequential File No.: 00187 File Date: 04/26/2008

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUH S3-0079
Control Solution %: 0.100% Expires: 02/20/2009
Solution Control Lot: 07B044 Bottle No.: 0702

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	18:18D		
Control 1 EC	0.100%	18:19D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	18:19D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:19D		
Control 2 EC	0.099%	18:20D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	18:20D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:20D		
Control 3 EC	0.100%	18:21D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	18:21D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:22D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: ROGERS

First Name: MICHAEL

MI: J

Signature: _____

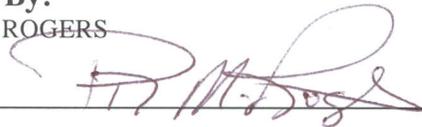

Badge No.: 258

Date: 04/26/2008

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARTL-0014
Location: SOUTH BRUNSWICK POLICE
Calibration File No.: 00163 Calib. Date: 09/21/2007 Calib. No.: 00007
Certification File No.: 00164 Cert. Date: 09/21/2007 Cert. No.: 00005
Linearity File No.: 00165 Lin. Date: 09/21/2007 Lin. No.: 00005
Solution File No.: 00186 Soln. Date: 03/31/2008 Soln. No.: 00043
Sequential File No.: 00186 File Date: 03/31/2008

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUH S3-0079
Control Solution %: 0.100% Expires: 02/20/2009
Solution Control Lot: 07B044 Bottle No.: 0713

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	11:53S		
Control 1 EC	0.100%	11:54S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.100%	11:54S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:54S		
Control 2 EC	0.100%	11:55S	33.9°C	*** TEST PASSED ***
Control 2 IR	0.100%	11:55S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:56S		
Control 3 EC	0.100%	11:56S	33.9°C	*** TEST PASSED ***
Control 3 IR	0.099%	11:56S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:57S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: ROGERS

First Name: MICHAEL

MI: J

Signature: _____



Badge No.: 258

Date: 03/31/2008

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARTL-0014
Location:	SOUTH BRUNSWICK POLICE	
Calibration File No.:	00163	Calib. Date: 09/21/2007
Certification File No.:	00164	Calib. No.: 00007
Linearity File No.:	00165	Cert. Date: 09/21/2007
Solution File No.:	00183	Cert. No.: 00005
Sequential File No.:	00183	Lin. Date: 09/21/2007
		Lin. No.: 00005
		Soln. Date: 03/07/2008
		Soln. No.: 00042
		File Date: 03/07/2008
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUH S3-0079
Solution Control Lot:	07B044	Expires: 02/20/2009
		Bottle No.: 0717

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	16:45S		
Control 1 EC	0.100%	16:45S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.100%	16:45S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:46S		
Control 2 EC	0.099%	16:46S	33.9°C	*** TEST PASSED ***
Control 2 IR	0.099%	16:46S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:47S		
Control 3 EC	0.099%	16:48S	33.9°C	*** TEST PASSED ***
Control 3 IR	0.100%	16:48S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:48S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: ROGERS

First Name: MICHAEL

MI: J

Signature: _____



Badge No.: 258

Date: 03/07/2008

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARTL-0014
Location:	SOUTH BRUNSWICK POLICE	Calib. No.:	00007
Calibration File No.:	00163	Calib. Date:	09/21/2007
Certification File No.:	00164	Cert. Date:	09/21/2007
Linearity File No.:	00165	Lin. Date:	09/21/2007
Solution File No.:	00181	Soln. Date:	02/07/2008
Sequential File No.:	00181	File Date:	02/07/2008
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUH S3-0079
Solution Control Lot:	07B044	Expires:	02/20/2009
		Bottle No.:	0723

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	15:27S		
Control 1 EC	0.101%	15:27S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	15:27S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:28S		
Control 2 EC	0.100%	15:29S	33.9°C	*** TEST PASSED ***
Control 2 IR	0.101%	15:29S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:29S		
Control 3 EC	0.100%	15:30S	33.9°C	*** TEST PASSED ***
Control 3 IR	0.100%	15:30S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:31S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: ROGERS

First Name: MICHAEL

MI: J

Signature: _____



Badge No.: 258

Date: 02/07/2008