

# Calibrating Unit New Standard Solution Report

**Equipment** Alcotest 7110 MKIII-C Serial No.: ARTL-0014  
Location: SOUTH BRUNSWICK POLICE  
Calibration File No.: 00346 Calib. Date: 12/26/2012 Calib. No.: 00024  
Certification File No.: 00347 Cert. Date: 12/26/2012 Cert. No.: 00016  
Linearity File No.: 00348 Lin. Date: 12/26/2012 Lin. No.: 00016  
Solution File No.: 00361 Soln. Date: 03/15/2013 Soln. No.: 00122  
Sequential File No.: 00361 File Date: 03/15/2013

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUH S3-0079  
Control Solution %: 0.100% Expires: 06/28/2014  
Solution Control Lot: 12F102 Bottle No.: 0414

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	07:59S		
Control 1 EC	0.098%	08:00S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.099%	08:00S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:00S		
Control 2 EC	0.098%	08:01S	33.9°C	*** TEST PASSED ***
Control 2 IR	0.099%	08:01S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:02S		
Control 3 EC	0.097%	08:02S	33.9°C	*** TEST PASSED ***
Control 3 IR	0.098%	08:02S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:03S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


## Changed By:

Last Name: DROST

First Name: KENNETH

MI: J

Signature: \_\_\_\_\_

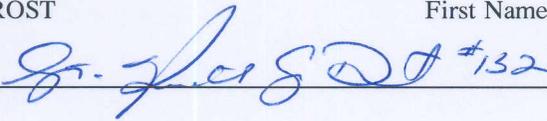

Badge No.: 132

Date: 03/15/2013