

# Calibrating Unit

## New Standard Solution Report

**Equipment** Alcotest 7110 MKIII-C Serial No.: ARTL-0014  
Location: SOUTH BRUNSWICK POLICE  
Calibration File No.: 00305 Calib. Date: 08/26/2011 Calib. No.: 00021  
Certification File No.: 00306 Cert. Date: 08/26/2011 Cert. No.: 00013  
Linearity File No.: 00307 Lin. Date: 08/26/2011 Lin. No.: 00013  
Solution File No.: 00310 Soln. Date: 10/20/2011 Soln. No.: 00095  
Sequential File No.: 00310 File Date: 10/20/2011

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUH S3-0079  
Control Solution %: 0.100% Expires: 12/16/2012  
Solution Control Lot: 10L084 Bottle No.: 0137

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	09:41D		
Control 1 EC	0.100%	09:41D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	09:41D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:42D		
Control 2 EC	0.100%	09:43D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.103%	09:43D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:43D		
Control 3 EC	0.101%	09:44D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.103%	09:44D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:44D		

All tests within acceptable tolerance.

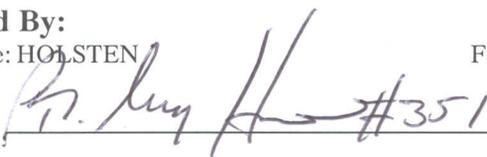
On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

### Changed By:

Last Name: HOLSTEN

First Name: GARY

MI: W

Signature:  #351

Badge No.: 351

Date: 10/20/2011