

Alcotest 7110 Calibration Record

Equipment


Alcotest 7110 MKIII-C	Serial No.:	ARTL-0014
Location: SOUTH BRUNSWICK POLICE		
Calibration File No.: 00546	Calib. Date: 01/14/2019	Calib. No.: 00040
Certification File No.: 00538	Cert. Date: 09/05/2018	Cert. No.: 00030
Linearity File No.: 00539	Lin. Date: 09/05/2018	Lin. No.: 00030
Solution File No.: 00545	Soln. Date: 01/02/2019	Soln. No.: 00214
Sequential File No.: 00546	File Date: 01/14/2019	
Calibrating Unit: WET	Model No.: CU-34	Serial No.: DDUH S3-0079
Control Solution %: 0.100%		Expires: 08/07/2019
Solution Control Lot: 17230		Bottle No.: 0148

Coordinator

Last Name: MIMIKOS	First Name: NICHOLAS	MI: E.
Signature: <u>TPR. N. A. #7413</u>	Badge No.: 7413	Date: 01/14/2019

*Black Key Temperature Probe Serial.....# DDEE P2-099

*Digital NIST Temperature Measuring System Serial.....# 170428357

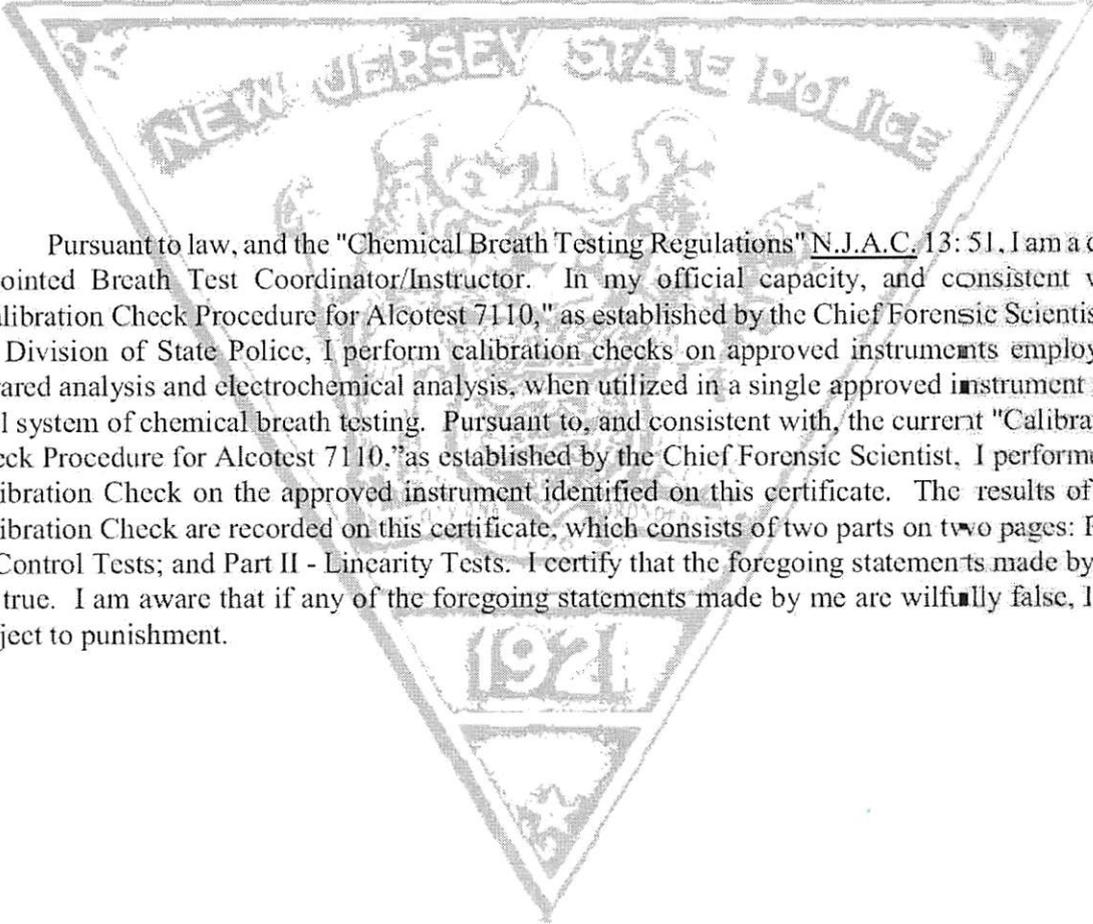

Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13: 51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis, when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to, and consistent with, the current "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.

Alcotest 7110 Calibration Certificate

Part I - Control Tests

Equipment Alcotest 7110 MKIII-C Serial No.: ARTL-0014
Location: SOUTH BRUNSWICK POLICE
Calibration File No.: 00546 Calib. Date: 01/14/2019 Calib. No.: 00040
Certification File No.: 00547 Cert. Date: 01/14/2019 Cert. No.: 00031
Linearity File No.: 00539 Lin. Date: 09/05/2018 Lin. No.: 00030
Solution File No.: 00545 Soln. Date: 01/02/2019 Soln. No.: 00214
Sequential File No.: 00547 File Date: 01/14/2019

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUH S3-0079
Control Solution %: 0.100% Expires: 08/07/2019
Solution Control Lot: 17230 Bottle No.: 0148

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	08:20S		
Control 1 EC	0.100%	08:21S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.099%	08:21S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:22S		
Control 2 EC	0.098%	08:22S	33.9°C	*** TEST PASSED ***
Control 2 IR	0.100%	08:22S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:23S		
Control 3 EC	0.098%	08:24S	33.9°C	*** TEST PASSED ***
Control 3 IR	0.100%	08:24S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:25S		

All tests within acceptable tolerance.

Coordinator

Last Name: MIMIKOS First Name: NICHOLAS MI: E.
Signature: TPR. N. A. #7413 Badge No.: 7413
Date: 01/14/2019

Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13: 51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis, when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to, and consistent with, the current "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.

Alcotest 7110 Calibration Certificate

Part II - Linearity Tests

Equipment Alcotest 7110 MKIII-C Serial No.: ARTL-0014
Location: SOUTH BRUNSWICK POLICE
Calibration File No.: 00546 Calib. Date: 01/14/2019 Calib. No.: 00040
Certification File No.: 00547 Cert. Date: 01/14/2019 Cert. No.: 00031
Linearity File No.: 00548 Lin. Date: 01/14/2019 Lin. No.: 00031
Solution File No.: 00545 Soln. Date: 01/02/2019 Soln. No.: 00214
Sequential File No.: 00548 File Date: 01/14/2019

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDRK S3-0021
Control Solution %: 0.040% Expires: 08/10/2019
Solution Control Lot: 17240 Bottle No.: 0144

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDRK S3-0022
Control Solution %: 0.080% Expires: 08/15/2019
Solution Control Lot: 17250 Bottle No.: 1256

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDSC S3-0013
Control Solution %: 0.160% Expires: 08/21/2019
Solution Control Lot: 17260 Bottle No.: 1029

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	08:38S		
Control 1 EC	0.043%	08:38S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.039%	08:38S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:40S		
Control 2 EC	0.043%	08:41S	33.9°C	*** TEST PASSED ***
Control 2 IR	0.040%	08:41S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:42S		
Control 3 EC	0.083%	08:43S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.080%	08:43S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:45S		
Control 4 EC	0.081%	08:45S	33.9°C	*** TEST PASSED ***
Control 4 IR	0.080%	08:45S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:47S		
Control 5 EC	0.162%	08:47S	33.9°C	*** TEST PASSED ***
Control 5 IR	0.159%	08:47S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:49S		
Control 6 EC	0.161%	08:50S	33.9°C	*** TEST PASSED ***
Control 6 IR	0.161%	08:50S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:51S		

All tests within acceptable tolerance.

Coordinator

Last Name: MIMIKOS

First Name: NICHOLAS

MI: E.

Signature: _____

TPR. N. A. #7413

Badge No.: 7413

Date: 01/14/2019

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARTL-0014
Location:	SOUTH BRUNSWICK POLICE		
Calibration File No.:	00546	Calib. Date:	01/14/2019
Certification File No.:	00547	Cert. Date:	01/14/2019
Linearity File No.:	00548	Lin. Date:	01/14/2019
Solution File No.:	00549	Soln. Date:	01/14/2019
Sequential File No.:	00549	File Date:	01/14/2019
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUH S3-0079
Solution Control Lot:	18150	Expires:	05/10/2020
		Bottle No.:	1121

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	09:57S		
Control 1 EC	0.102%	09:58S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.100%	09:58S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:59S		
Control 2 EC	0.100%	09:59S	33.9°C	*** TEST PASSED ***
Control 2 IR	0.100%	09:59S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:00S		
Control 3 EC	0.101%	10:01S	33.9°C	*** TEST PASSED ***
Control 3 IR	0.101%	10:01S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:02S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Temperature Probe Serial Number: DDSF P2-0394 A

Changed By:

Last Name: MIMIKOS	First Name: NICHOLAS	MI: E.
Signature: <u>TPR. N.A. #7413</u>	Badge No.: 7413	Date: 01/14/2019

Dräger

Alcotest® 7110 MKIII-C

CERTIFICATE OF ACCURACY

This is to certify that the Alcotest 7110 MKIII-C has been tested for accuracy and found to be in compliance with the National Highway Traffic Safety Administration Standard for roadside breath testing devices. The Alcotest MKIII-C is compliant as a "mobile" and "nonmobile" EBT with 49 FR 48254, 49 FR 48864 and 53 FR 48705. The manufacturer recommends accuracy verification of this instrument within 12 months of the calibration date below, or sooner, according to your State Specifications.

Certification Date:

4-16-15

SERIAL NUMBER:

ARTZ-0014

Dräger Safety Diagnostics, Inc.

BC



Calibration
Certificate No. 1750.01

Calibration complies with ISO/IEC
17025, ANSI/NCSL Z540-1, and 9001



Cert. No.: 4000-8609157

Traceable® Certificate of Calibration for Digital Thermometer

Manufactured for and distributed by: VWR International, LLC, Radnor Corporate Center, Bldg 1, Ste 200, 100 Matsonford Road, Radnor, PA 19087

Instrument Identification:

Model: 61220-601 S/N: 170428357 Manufacturer: Control Company

Standards/Equipment:

Description	Serial Number	Due Date	NIST Traceable Reference
Temperature Calibration Bath TC-231	A79341		
Thermistor Module	A27129	12/01/17	1000401760
Temperature Probe	5267	12/06/17	B6B30059
Temperature Calibration Bath TC-191	A42238		
Thermistor Module	A27129	12/01/17	1000401760
Temperature Probe	5202	12/19/17	B6B30058-1
Temperature Calibration Bath TC-218	A73332		
Thermistor Probe	5356	1/10/18	B7104024
Readout, Digital Thermometer	B5C344	3/12/18	B7314035
Temperature Calibration Bath TC-275	B16388		
Thermistor Probe	5357	1/06/18	B7104023
Readout, Digital Thermometer	B5C344	3/12/18	B7314035

Certificate Information:

Technician: 104 Procedure: CAL-06 Cal Date: 6/08/17 Due Date: 6/08/19
Test Conditions: 23.5°C 50.0 %RH 1014 mBar

Calibration Data: (New Instrument)

Unit(s)	Nominal	As Found	In Tol	Nominal	As Left	In Tol	Min	Max	±U	TUR
°C		N.A.		0.002	0.000	Y	-0.048	0.052	0.010	>4:1
°C		N.A.		25.003	25.002	Y	24.953	25.053	0.010	>4:1
°C		N.A.		50.002	50.000	Y	49.952	50.052	0.010	>4:1
°C		N.A.		100.001	100.000	Y	99.951	100.051	0.010	>4:1

This instrument was calibrated using instruments traceable to National Institute of Standards and Technology.

A Test Uncertainty Ratio of at least 4:1 is maintained unless otherwise stated and is calculated using the expanded measurement uncertainty. Uncertainty evaluation includes the instrument under test and is calculated in accordance with the ISO "Guide to the Expression of Uncertainty in Measurement" (GUM). The uncertainty represents an expanded uncertainty using a coverage factor k=2 to approximate a 95% confidence level. In tolerance conditions are based on test results falling within specified limits with no reduction by the uncertainty of the measurement. The results contained herein relate only to the item calibrated. This certificate shall not be reproduced except in full, without written approval of Control Company.

Nominal=Standard's Reading; As Left=Instrument's Reading; In Tol=In Tolerance; Min/Max=Acceptance Range; ±U=Expanded Measurement Uncertainty; TUR=Test Uncertainty Ratio; Accuracy= $\pm(\text{Max}-\text{Min})/2$; Min = As Left Nominal(Rounded) - Tolerance; Max = As Left Nominal(Rounded) + Tolerance; Date=MM/DD/YY

Nicol Rodriguez
Nicol Rodriguez, Quality Manager

Aaron Judice
Aaron Judice, Technical Manager

Maintaining Accuracy:

In our opinion once calibrated your Digital Thermometer should maintain its accuracy. There is no exact way to determine how long calibration will be maintained. Digital Thermometers change little, if any at all, but can be affected by aging, temperature, shock, and contamination.

Recalibration:

For factory calibration and re-certification traceable to National Institute of Standards and Technology contact Control Company.

CONTROL COMPANY 12554 Galveston RD Suite B230 Webster TX USA 77598
Phone 281 482-1714 Fax 281 482-9448 service@control3.com www.control3.com

Control Company is an ISO 17025:2005 Calibration Laboratory Accredited by (AZLA) American Association for Laboratory Accreditation, Certificate No. 1750.01.
Control Company is ISO 9001:2008 Quality Certified by (DNV) Det Norske Veritas, Certificate No. CERT-0180S-2008-AQ-HOU-RwA.
International Laboratory Accreditation Cooperation (ILAC) - Multilateral Recognition Arrangement (MRA).

Dräger

Simulator

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)
Dräger, Inc.

Model: ALCOTEST CU34

Model: MARK IIA

Other: _____

Serial Number:

DDRK 53-0021

Certification Date:

8-23-18

Technician:

BS

Re-Certification Due Date:

8-23-19

Dräger

Simulator

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)
Dräger, Inc.

Model: ALCOTEST CU34

Model: MARK IIA

Other: _____

Serial Number:

DDRK 53-0022

Certification Date:

8-23-18

Technician:

BS

Re-Certification Due Date:

8-23-19

Dräger

Simulator

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)
Dräger, Inc.

- Model: ALCOTEST CU34
- Model: MARK IIA
- Other: _____

Serial Number:

DDSC53-0013

Certification Date:

8-23-18

Technician:

BS

Re-Certification Due Date:

8-23-19

Dräger

Alcotest 7110 Temperature Probe

CERTIFICATE OF ACCURACY

This is to certify that the Alcotest 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST). The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your state's specifications.
For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest 7110.

Serial Number Temp Probe:

DDEEP2-099

Certification Date:

8-23-18

Next Certification Due:

8-23-19

Probe Value:

103

Dräger, Inc.

BS

Dräger

Simulator

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)
Draeger, Inc.

- Model: ALCOTEST CU34
- Model: MARK IIA
- Other: _____

Serial Number:

DDU453-0079

Certification Date:

12-14-18

Technician:

BS

Re-Certification Due Date:

12-14-19

Dräger

Alcotest 7110 Temperature Probe

CERTIFICATE OF ACCURACY

This is to certify that the Alcotest 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST). The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your state's specifications. For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest 7110.

Serial Number Temp Probe:

DDSE P2-D394

Certification Date:

12-13-18

Next Certification Due:

12-13-19

Probe Value:

103

Draeger, Inc.

BS



State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

CHRIS CHRISTIE
Governor

KIM GUADAGNO
Lt. Governor

CHRISTOPHER S. PORRINO
Attorney General

COLONEL JOSEPH R. FUENTES
Superintendent

CERTIFICATION OF ANALYSIS
0.10 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.1174 to 0.1246 grams per 100 milliliters of solution.

MANUFACTURER: Draeger Safety, Inc.

ANALYSIS DATE: 08/24/2017

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 17230

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1202 to 0.1216 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is August 07, 2019.


As Research Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

[Handwritten signature of Ali M. Alaouie]

Ali M. Alaouie, Ph.D.
Research Scientist
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 24 day of August, 2017.

[Handwritten signature of Notary]
Notary

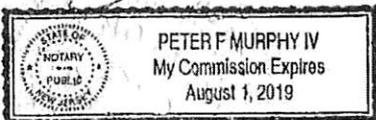

"An Internationally Accredited Agency"

New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable





State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

CHRIS CHRISTIE
Governor
KIM GUADAGNO
Lt. Governor

CHRISTOPHER S. PORRINO
Attorney General
COLONEL JOSEPH R. FUENTES
Superintendent

CERTIFICATION OF ANALYSIS
0.04 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.0469 to 0.0499 grams per 100 milliliters of solution.

MANUFACTURER: Draeger Safety, Inc.

ANALYSIS DATE: 08/29/2017

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 17240

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.0483 to 0.0489 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is August 10, 2019.

As Research Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

[Handwritten signature of Ali M. Alaouie]

Ali M. Alaouie, Ph.D.
Research Scientist
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 30th day of August, 2017.

[Handwritten signature of Mary Elizabeth McLaughlin]
Notary

MARY ELIZABETH MCLAUGHLIN
ID # 2052190
NOTARY PUBLIC
STATE OF NEW JERSEY
My Commission Expires Dec. 24, 2018



"An Internationally Accredited Agency"

New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable





State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

CHRIS CHRISTIE
Governor

KIM GUADAGNO
Lt. Governor

CHRISTOPHER S. PORRINO
Attorney General

COLONEL JOSEPH R. FUENTES
Superintendent

CERTIFICATION OF ANALYSIS
0.08 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.0939 to 0.0997 grams per 100 milliliters of solution.

MANUFACTURER: Draeger Safety, Inc.

ANALYSIS DATE: 09/07/2017

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 17250

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.0963 to 0.0973 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is August 15, 2019.

As Research Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

[Signature]
Ali M. Alaouie, Ph.D.
Research Scientist
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 11 day of September, 2017.

[Signature]
Notary

PETER F. MURPHY IV
My Commission Expires
August 1, 2019



"An Internationally Accredited Agency"
New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable





State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

CHRIS CHRISTIE
Governor
KIM GUADAGNO
Lt. Governor

CHRISTOPHER S. PORRINO
Attorney General
COLONEL JOSEPH R. FUENTES
Superintendent

CERTIFICATION OF ANALYSIS
0.16 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.1878 to 0.1994 grams per 100 milliliters of solution.

MANUFACTURER: Draeger Safety, Inc. ANALYSIS DATE: 09/12/2017
BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 17260

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1937 to 0.1957 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is August 21, 2019.


As Research Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

[Handwritten signature]

Ali M. Alaouie, Ph.D.
Research Scientist
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 13 day of September, 2017.

[Handwritten signature]
Notary

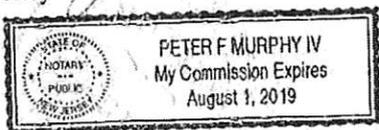

"An Internationally Accredited Agency"

New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable





State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

PHILIP D. MURPHY
Governor

SHEILA Y. OLIVER
Lt. Governor

GURBIR S. GREWAL
Attorney General

PATRICK J. CALLAHAN
Colonel

CERTIFICATION OF ANALYSIS
0.10 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.1174 to 0.1246 grams per 100 milliliters of solution.

MANUFACTURER: Draeger Safety, Inc.

ANALYSIS DATE: 05/24/2018

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 18150

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1212 to 0.1239 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is May 10, 2020.


As Research Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

[Handwritten signature of Ali M. Alaouie]

Ali M. Alaouie, Ph.D.
Research Scientist
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 29th day of May, 2018.

[Handwritten signature of Notary]
Notary

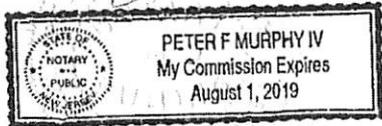

"An Internationally Accredited Agency"

New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable



DEPARTMENT OF
Traffic and Public Safety
Works to be certified Dept

NICHOLAS E. MIMIKOS
NEW JERSEY STATE POLICE

IS QUALIFIED AND COMPETENT TO CONDUCT THE TEST AND ISSUES PERMITS TO CHAPTER 142 OF
 THE LAWS OF NEW JERSEY IN THE OPERATION OF THE **ALCOHOL TEST 7110 MKIII-C**
 A METER TO DETERMINE BLOOD ALCOHOL CONTENT
 GIVEN UNDER MY HAND AND THE SEAL OF THE STATE ON THIS 23rd DAY OF **OCTOBER**

TWO THOUSAND AND **FOURTEEN**

[Signature]
 DEPARTMENT CHIEF
 NEW JERSEY STATE POLICE

[Signature]
 DEPUTY ATTORNEY GENERAL
 STATE OF NEW JERSEY

ORIGINAL COURSE DATES

DATE	Refresh Course PLACE	INSTRUCTOR
1. <u>6-3-16</u>	<u>PERLEN CPA</u>	<u>[Signature]</u>
2. <u>1-19-18</u>	<u>PERLEN CPA</u>	<u>[Signature]</u>
3. _____	_____	_____
4. _____	_____	_____
5. _____	_____	_____
6. _____	_____	_____
7. _____	_____	_____
8. _____	_____	_____
9. _____	_____	_____

S.P. 2038 (REV. 08/13)

DEPARTMENT OF
Traffic and Public Safety
 This is to certify that

Nicholas E. Mimikos

Breath Test Coordinator/Instructor

IS QUALIFIED AND COMPETENT TO CONDUCT MEDICAL BREATH ANALYSES PURSUANT TO CHAPTER 141 OF
 THE LAWS OF 1966 IN THE OPERATION OF THE Alcotest 7110 MKIII-C
 A METHOD TO DETERMINE INTOXICATION
 GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY THIS 9th DAY OF October

TWO THOUSAND AND Eighteen


 COLONEL
 NEW JERSEY STATE POLICE


 ATTORNEY GENERAL
 STATE OF NEW JERSEY

ORIGINAL COURSE DATES _____

DATE	Refresher Course PLACE	INSTRUCTOR
1.	_____	_____
2.	_____	_____
3.	_____	_____
4.	_____	_____
5.	_____	_____
6.	_____	_____
7.	_____	_____
8.	_____	_____
9.	_____	_____

S.P. 283B (Rev. 01/18)