

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARNK-0074
Location:	SOUTH BRUNSWICK POLICE	
Calibration File No.:	01008	Calib. Date: 01/14/2019
Certification File No.:	01009	Calib. No.: 00041
Linearity File No.:	01010	Cert. Date: 01/14/2019
Solution File No.:	01026	Cert. No.: 00029
Sequential File No.:	01026	Lin. Date: 01/14/2019
		Lin. No.: 00029
		Soln. Date: 03/13/2019
		Soln. No.: 00222
		File Date: 03/13/2019
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUF S3-0061
Solution Control Lot:	18150	Expires: 05/10/2020
		Bottle No.: 1175

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	09:01S		
Control 1 EC	0.099%	09:02S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	09:02S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:03S		
Control 2 EC	0.099%	09:03S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	09:03S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:04S		
Control 3 EC	0.100%	09:05S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	09:05S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:05S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


**Changed By:**

Last Name: HOLSTEN

First Name: GARY

MI: W

Signature: \_\_\_\_\_

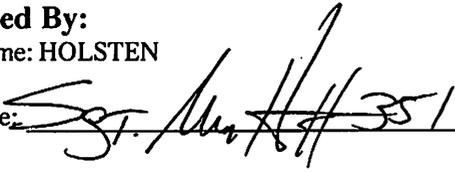

Badge No.: 351

Date: 03/13/2019